

STERILIZATION PROGRAMS, AIR REMOVAL AND STEAM PENETRATION

Peter Hooper CEng MIMechE FIHEEM, United Kingdom

Sterilization Programs, Air Removal and Steam Penetration

Agenda:

How steam sterilization works

Why air is a problem

How is air removed

What are the effects of poor air removal

Different cycle types

Monitoring air removal

Sterilization Programs, Air Removal and Steam Penetration

Steam sterilization works by:

Using steam to transfer energy from the boiler/generator to the load in the sterilizer

The steam contains two packets of energy

1. that to raise its temperature from cold to boiling point
2. that to turn boiling water into steam at the same temperature

For each kilogram of steam energy 2 is approximately 4-5 times that of energy 1

When steam condenses energy 2 is given to the surface it condenses on – **this condensation is vital**

Sterilization Programs, Air Removal and Steam Penetration

Why is air a problem?

It inhibits the access of steam (and hence energy transfer) to ALL surfaces – *ie inhibits steam penetration*

It acts as an insulator to inhibit energy transfer

It mixes with the steam to destroy the fixed pressure/temperature relationship used to control the sterilizer

It is non-condensable and contains little energy to transfer

Thus AIR MUST BE REMOVED FROM THE ENTIRE CHAMBER

Sterilization Programs, Air Removal and Steam Penetration

A steam sterilizer cycle consists of:

Air removal – *the stage without which sterilization will not occur*

Heat-up

Sterilization – *the central 3 minutes of a 45-minute cycle*


Steam removal

Drying

Air inlet

How is air removed?


1. A long, deep vacuum at the start of the cycle?

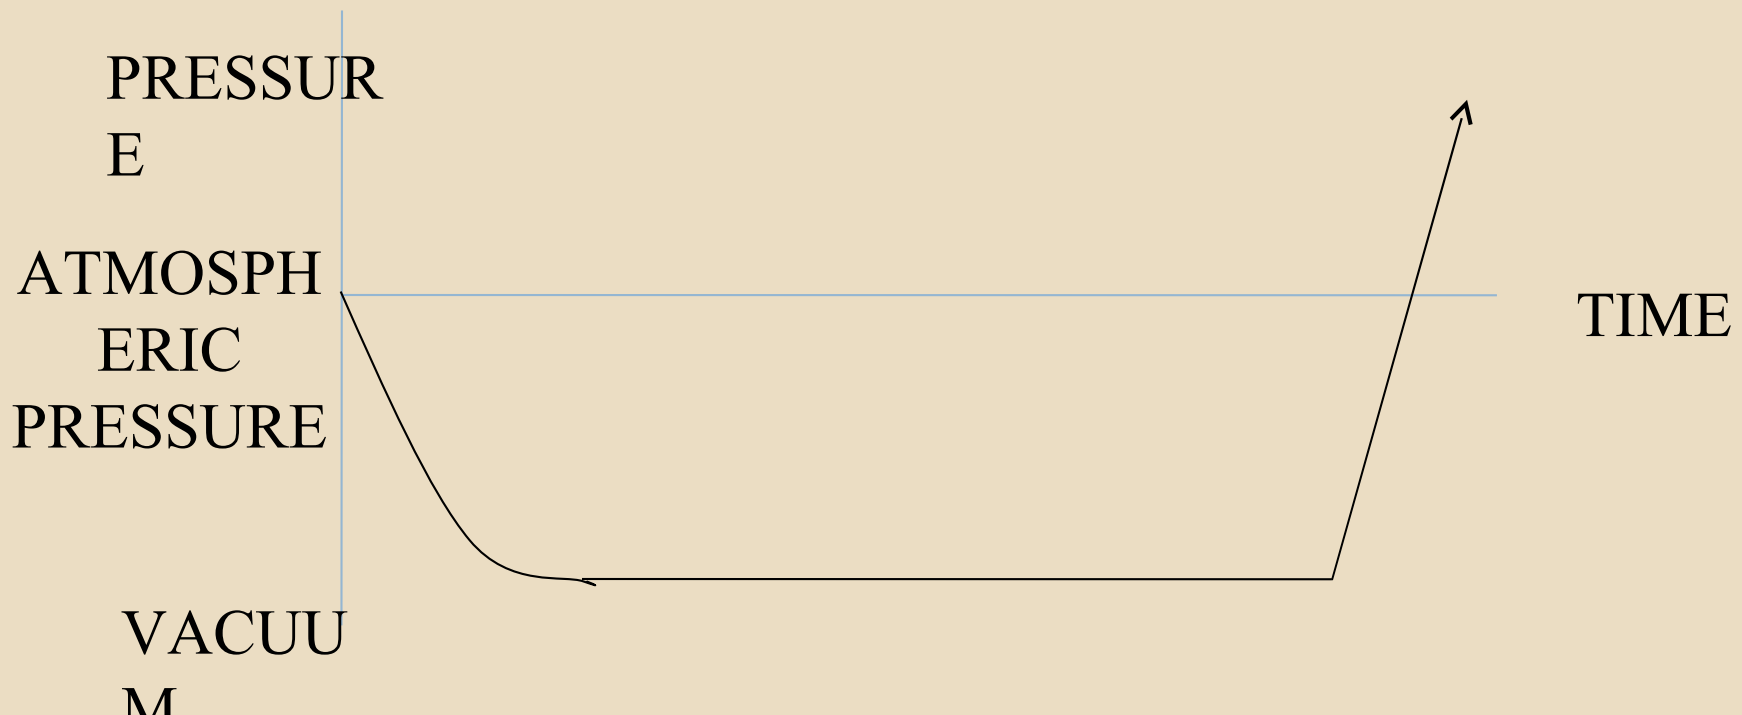

Sterilization Programs, Air Removal and Steam Penetration

How is air removed?

2. Pulsing

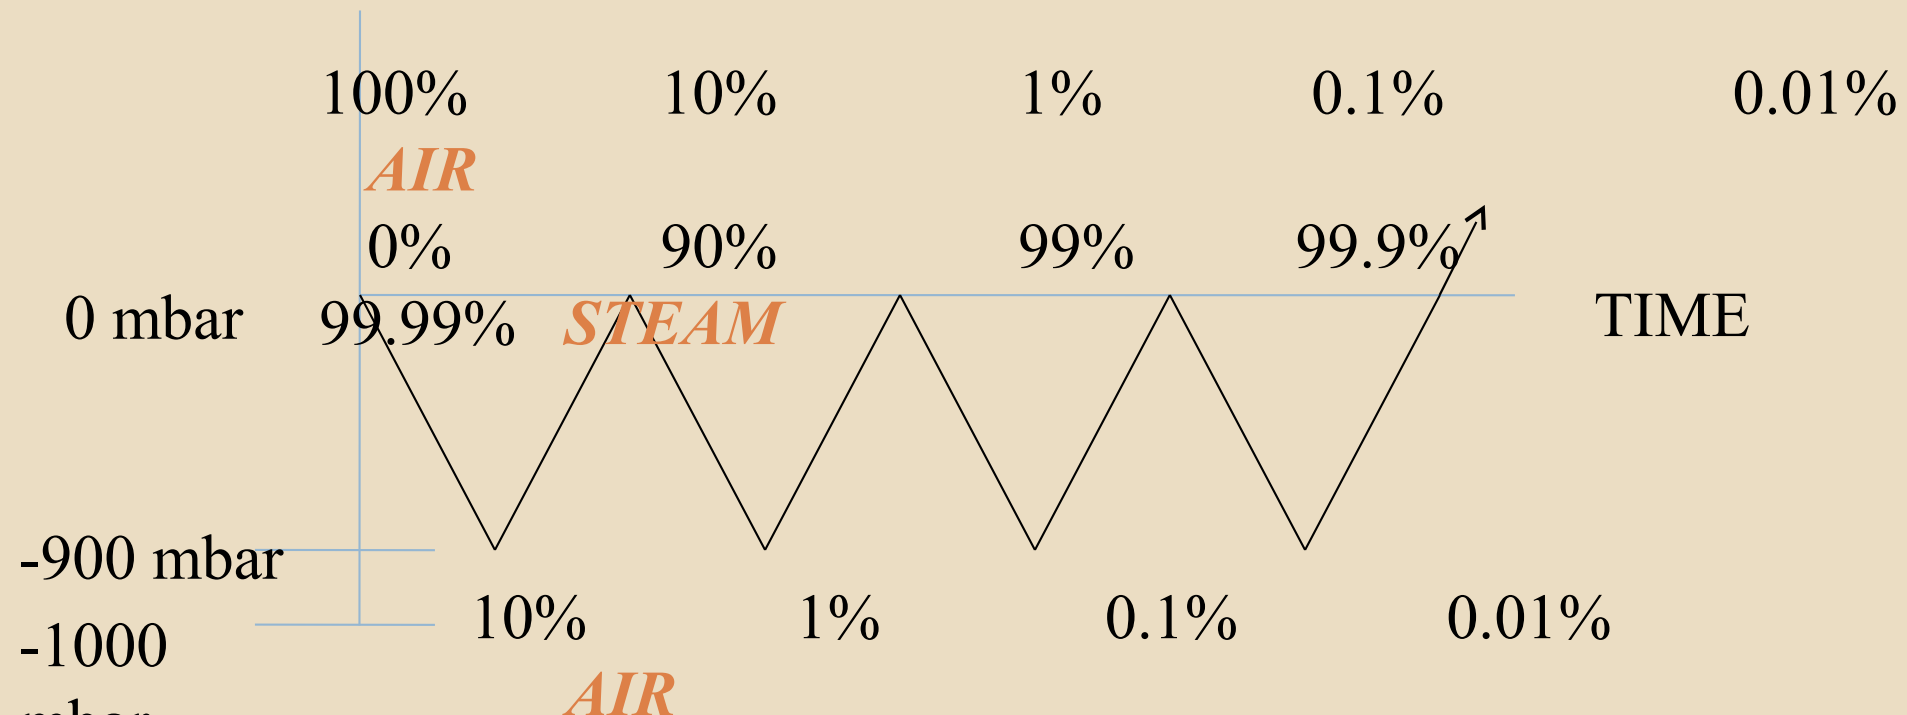

Sterilization Programs, Air Removal and Steam Penetration

Conclusion:

Pulsing is the most efficient method


The efficiency depends upon:

1. The number of pulses
2. The depth of each pulse

So which is the best pulsing system design?


Sterilization Programs, Air Removal and Steam Penetration

1

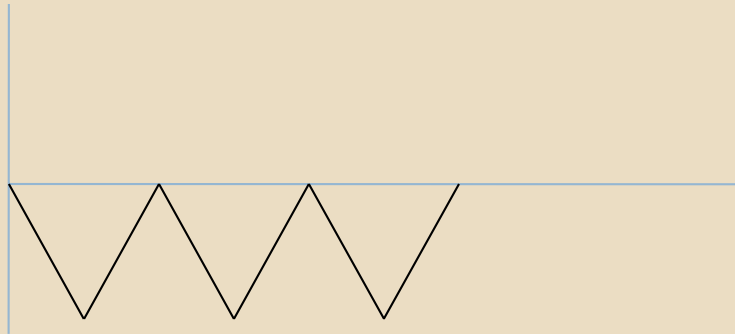


NEGATIVE

2

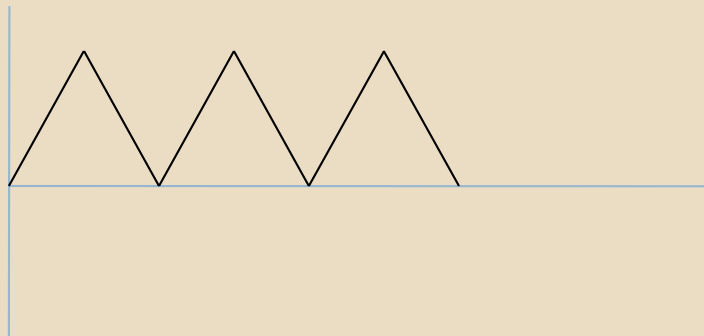

POSITIVE

3

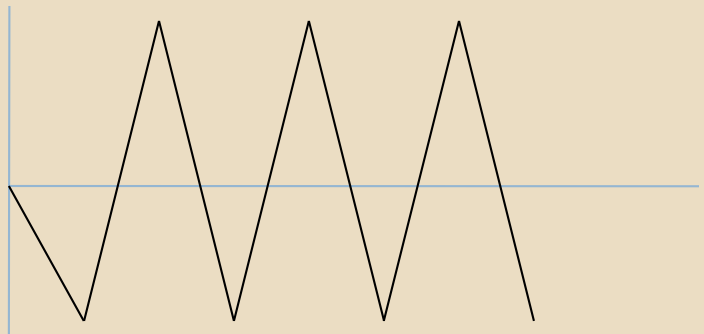

Sterilization Programs, Air Removal and Steam Penetration

Advantages & disadvantages:

Negative pulses

Can induce air through leaks

Positive pulses


Less efficient but no air ingress

Trans-atmospheric pulses

Most efficient but has negative sections


Sterilization Programs, Air Removal and Steam Penetration

A possible final cycle – a compromise:

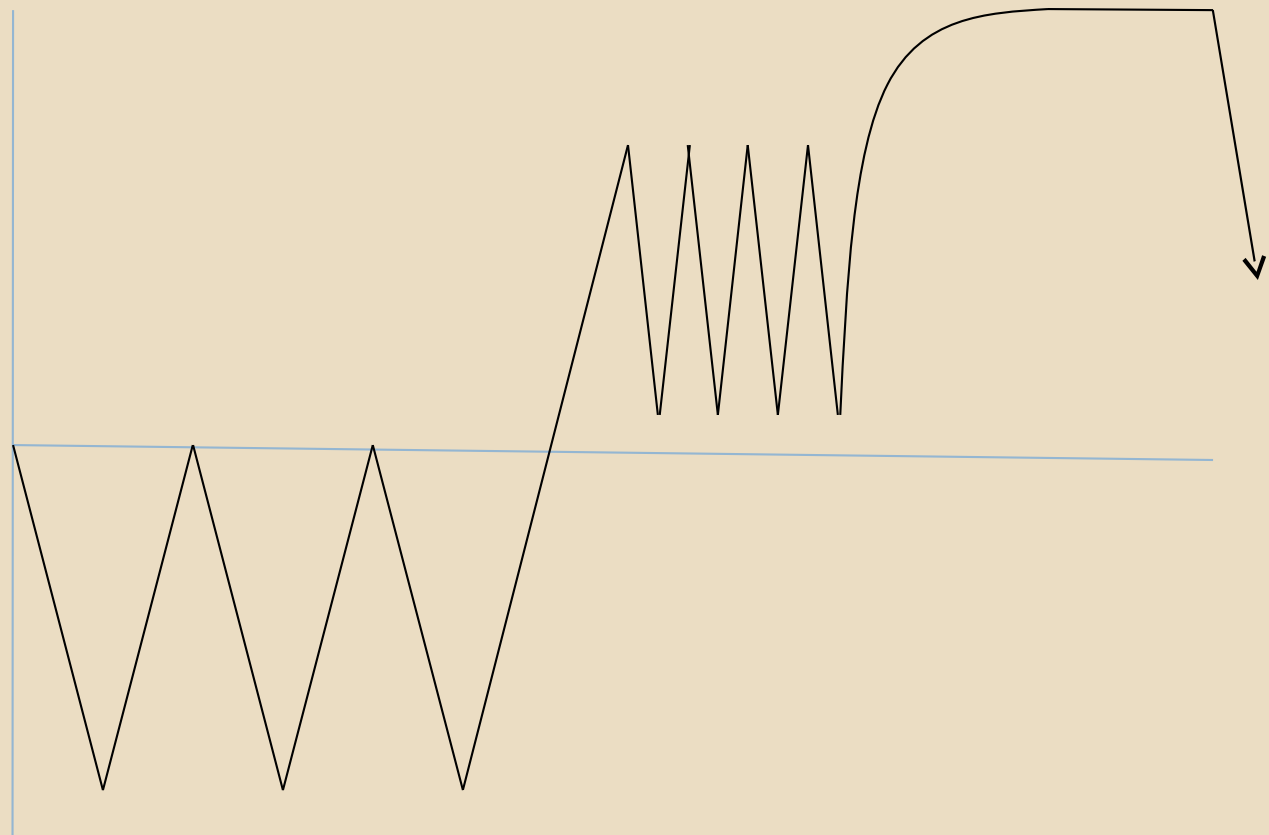

Sterilization Programs, Air Removal and Steam Penetration


Important points for air removal:

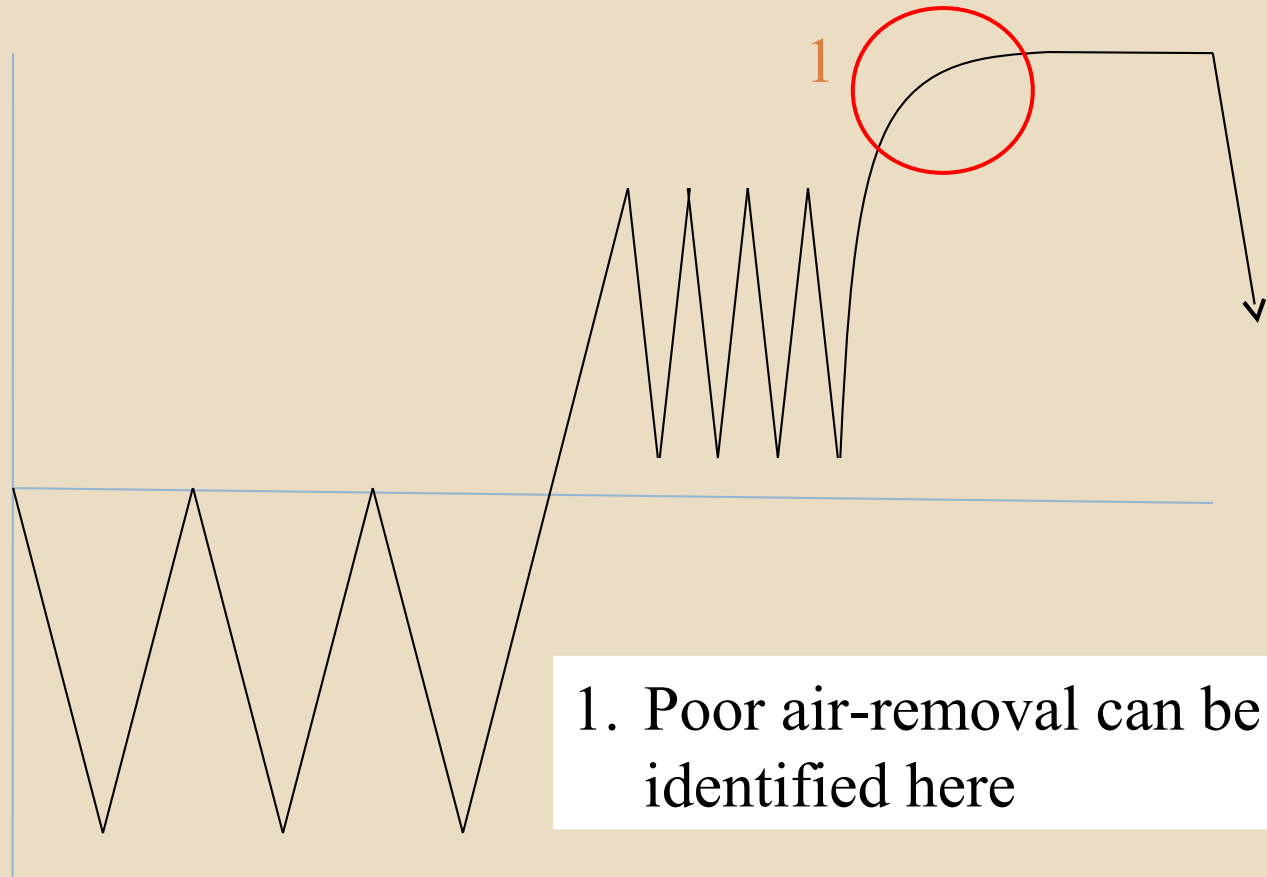

1. Poor air-removal can be identified here


Sterilization Programs, Air Removal and Steam Penetration

Measuring air-removal:

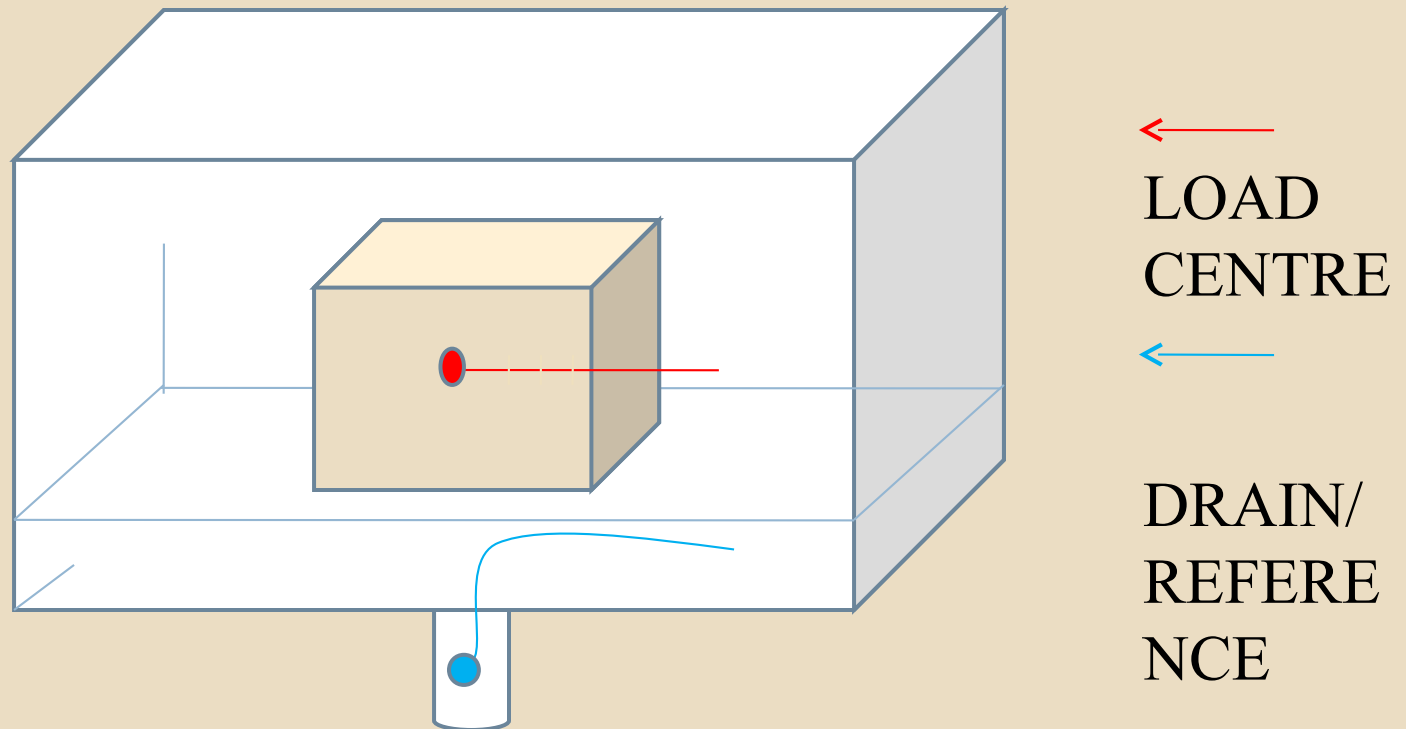


Sterilization Programs, Air Removal and Steam Penetration

Thermocouple traces: perfection

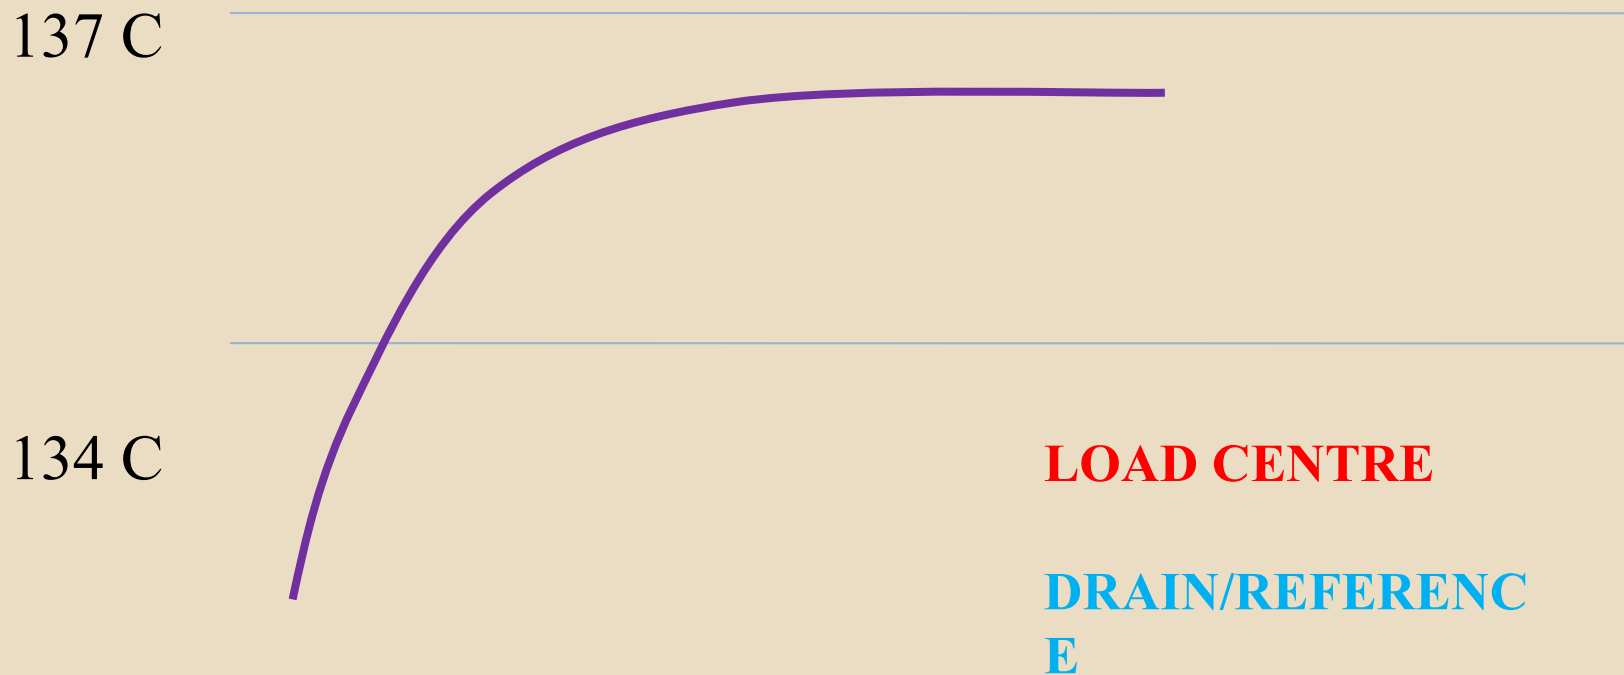


Sterilization Programs, Air Removal and Steam Penetration

Thermocouple traces: reality

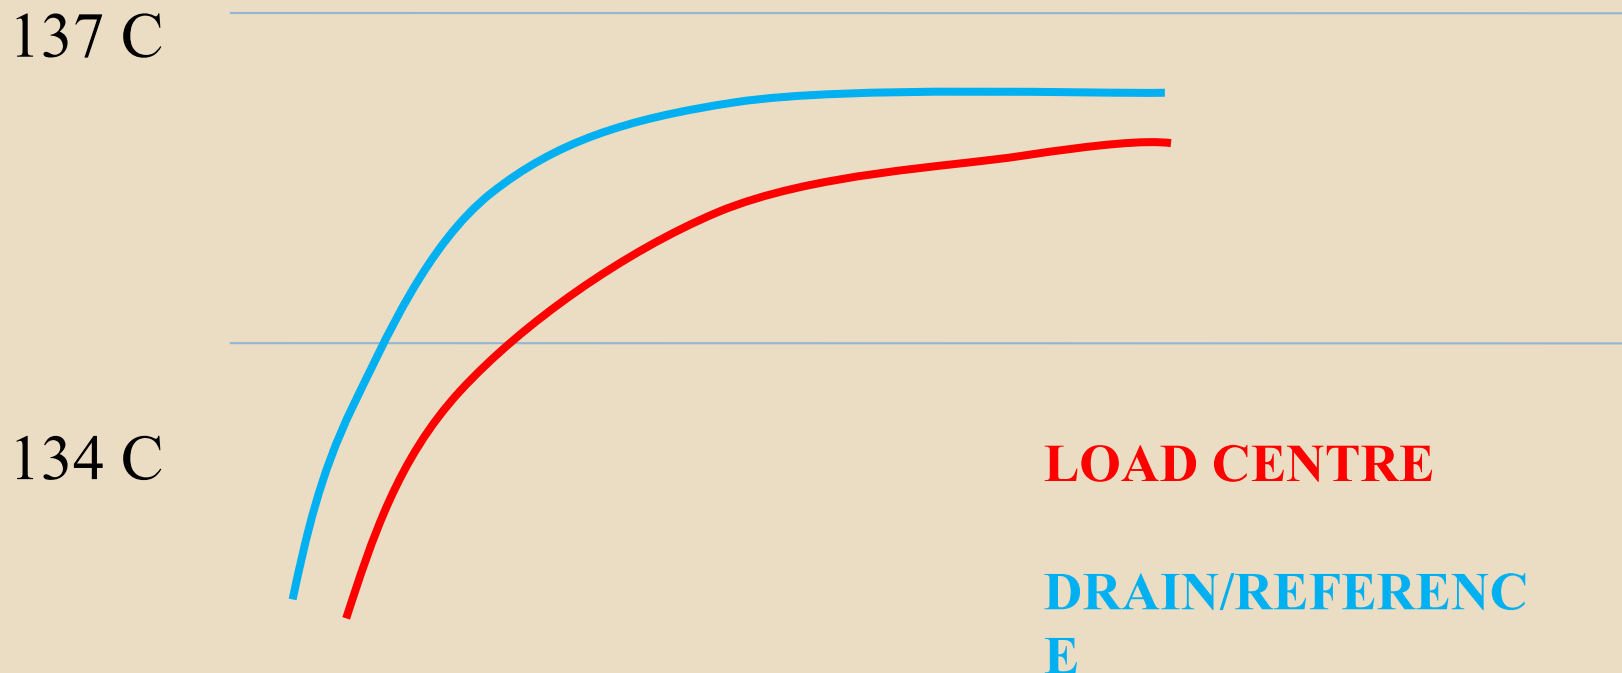


Sterilization Programs, Air Removal and Steam Penetration

Thermocouple traces:

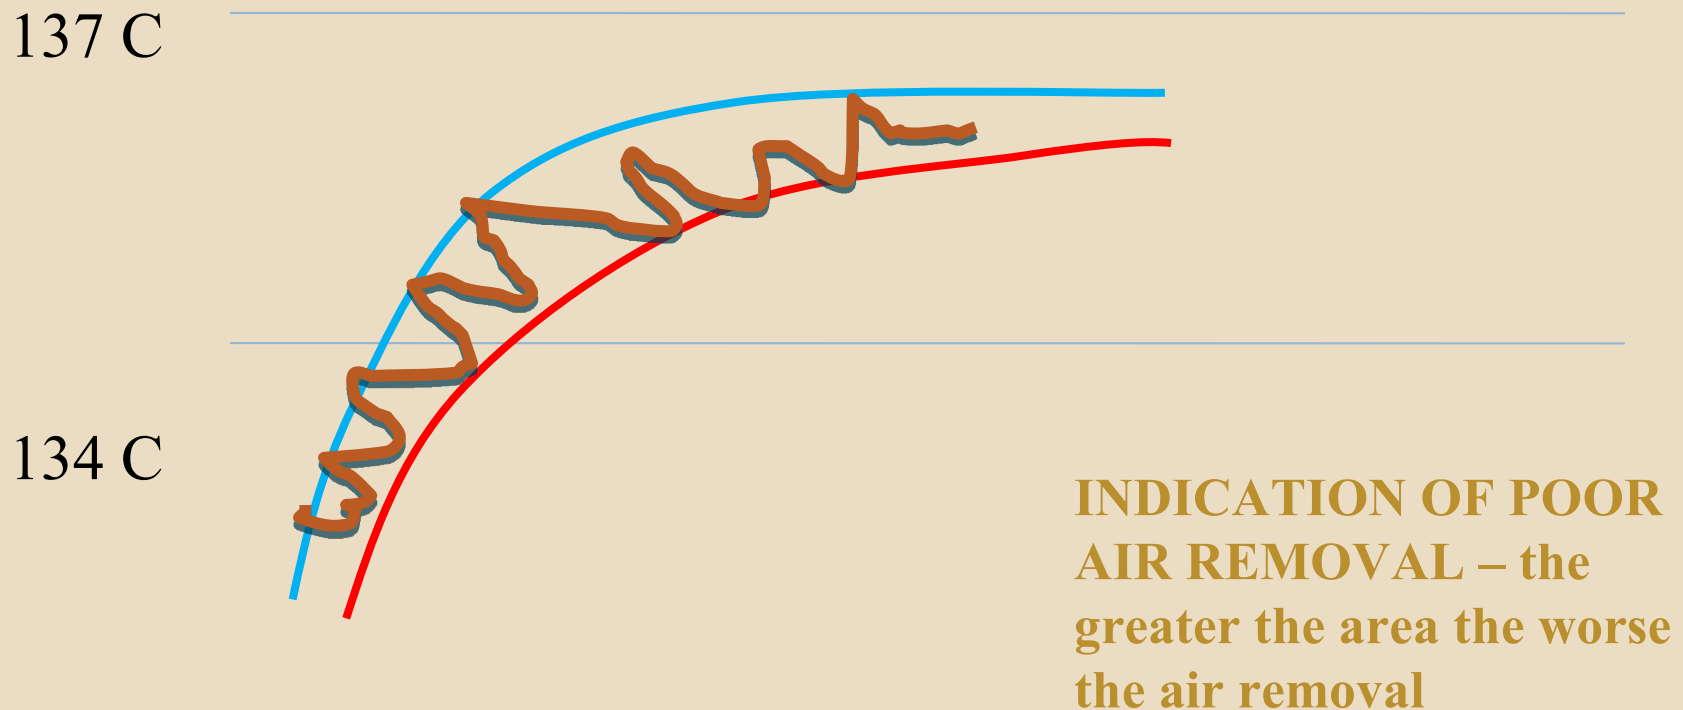


Sterilization Programs, Air Removal and Steam Penetration

Thermocouple traces:

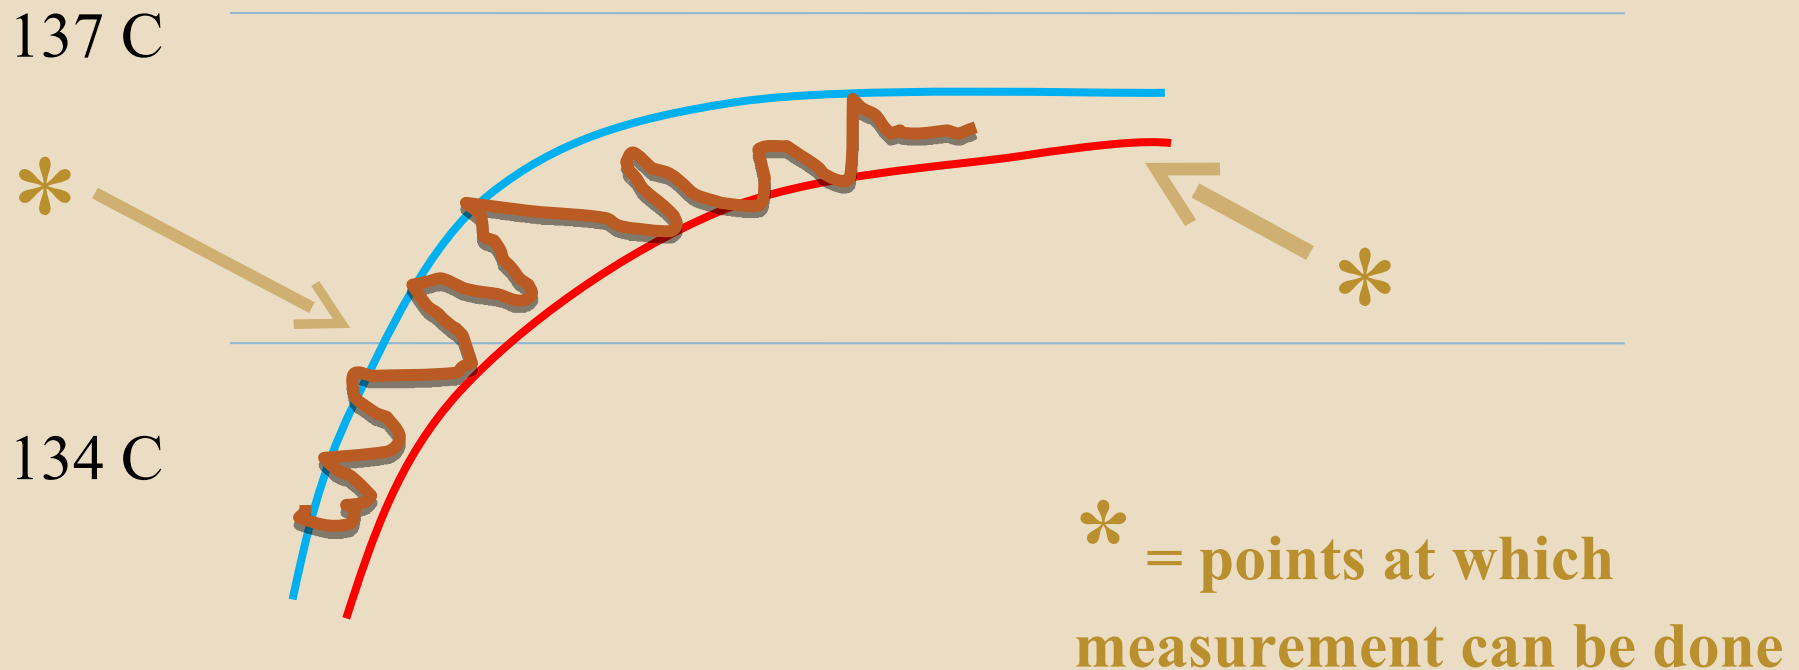

Sterilization Programs, Air Removal and Steam Penetration

Quantification of thermocouple traces:

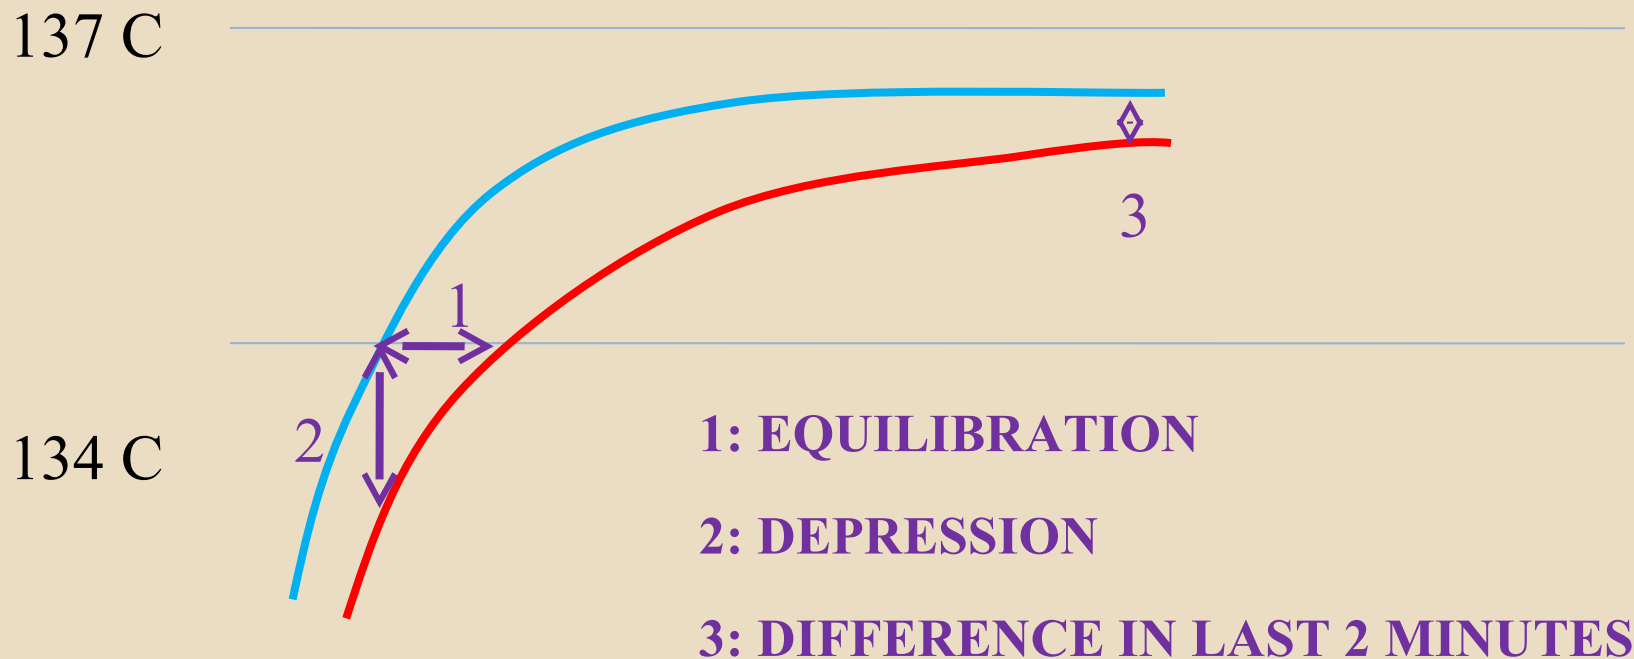

Quantification of thermocouple traces:



Sterilization Programs, Air Removal and Steam Penetration

Comparison of parameter values in the UK:

DOCUMENT	YEAR	1 equilibration	2 depression	3 difference
HTM 10	1968	-	-	-
HTM 10	1980	-	-	0
HTM 2010	1994	15	2*	2
EN 285 >>	1994 >>*	15 = for air detectors	2*	2

Air removal monitoring:

- Internal sensors and timers (control)
- Bowie & Dick test (daily test)
- Process Challenge devices (in-chamber in-cycle when used)
- Air detector (external in-cycle every cycle)

Sterilization Programs, Air Removal and Steam Penetration

Bowie & Dick test:

Initially defined with Standard Test Pack (textile)

Later quantified via Standards

Parameter definitions used to define failure chemistry

NOTE: parameter values and test pack details may differ in different parts of the World

Air detector:

- A device to automatically monitor the efficacy of the air-removal process – it can automatically fail the cycle if it measures unacceptable air removal
- It can function each cycle
- It is part of the control system, not an accessory
- It can abort cycles at an early stage of air-removal
 - ie it can be predictive
- It must be validated and periodically tested with care and skill
- It is extremely accurate and precise

Sterilization Programs, Air Removal and Steam Penetration

Air detector:

It works by sealing a sample of chamber contents and, by condensation caused by heat loss, separates residual air


The amount of air can be measured by either its partial pressure or temperature depression

It is part of the chamber but external to it to enable the heat loss to occur

A temperature-operated air detector can be predictive and can be used to monitor hold-time conditions

Sterilization Programs, Air Removal and Steam Penetration

Important points for air detector:

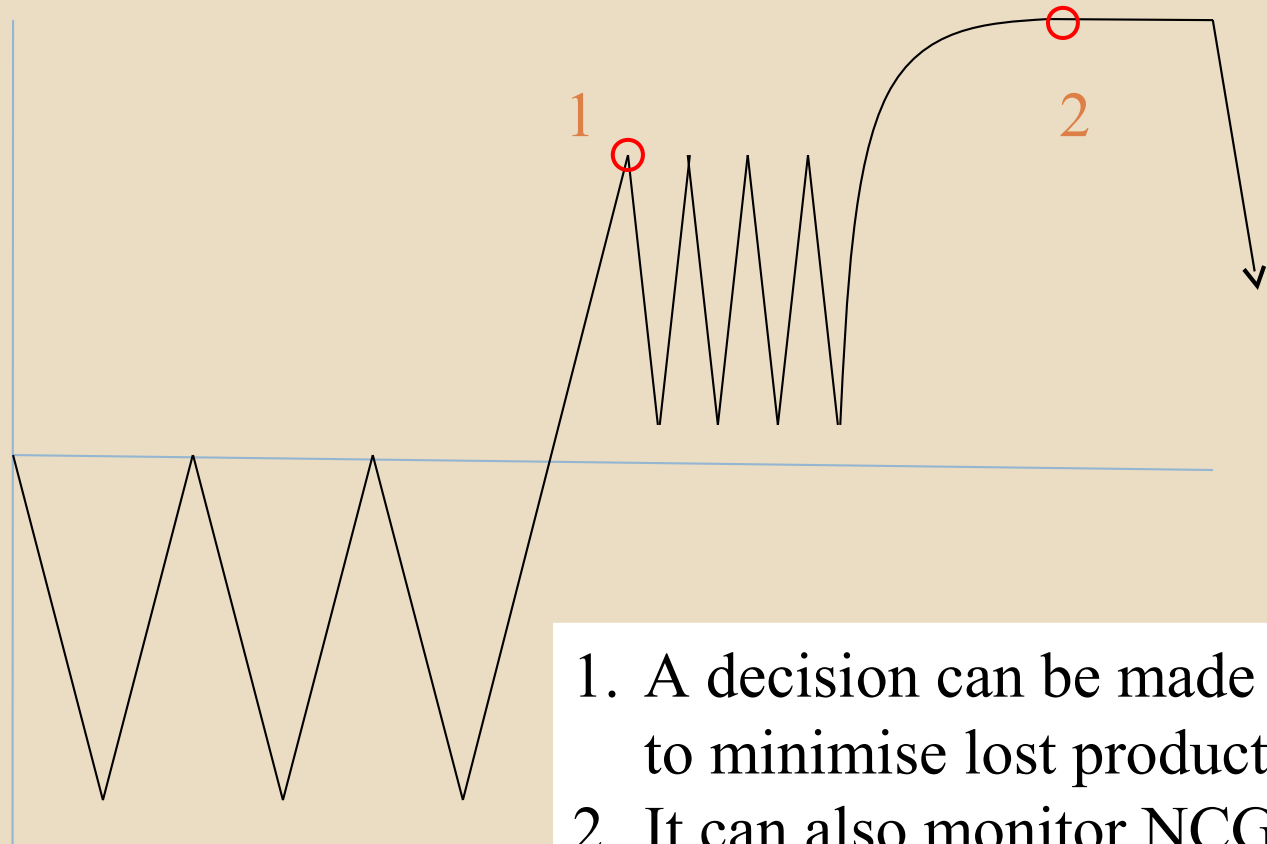

1. A decision can be made here to minimise lost productivity
2. It can also monitor NCG levels

Sterilization Programs, Air Removal and Steam Penetration

Summary:

- Complete air-removal is essential to good sterilization
- Pulsing is the most efficient method of air removal
- A variety of pulsing systems may be used – they each have benefits and disadvantages
- Poor air-removal can be shown by thermometric testing
- Thermometric data can be used to quantify air-removal and thus define performance of air-removal monitors
- Bowie & Dick test parameters can be thus defined but may differ from place to place
- An air-detector is an accurate and repeatable method of monitoring every process cycle



Thank you
σε ευχαριστώ